Development and optimization of an external-membrane introduction photoionization mass spectrometer for the fast analysis of (polycyclic)aromatic compounds in environmental and process waters.

CHRISTIAN GEHM[1], THORSTEN STREIBEL[1,2]*, SVEN EHLERT[4], DETLEF SCHULZ-BULL[3], RALF ZIMMERMANN[1,2]

[1]Joint Mass Spectrometry Centre, Chair of Analytical Chemistry, Institute of Chemistry, University of Rostock, Dr.-Lorenz-Weg 2, 18059 Rostock, Germany

[2]Joint Mass Spectrometry Centre, Cooperation Group Comprehensive Molecular Analytics, Institute of Ecological Chemistry, Helmholtz Zentrum München-German Research Center of Environmental Health (GmbH), Ingolstädter Landstrasse 1, 85764 Neuherberg, Germany

[3]Leibniz - Institute for Baltic Sea Research Warnemünde, Seestraße 15, 18119 Rostock – Warnemünde, Germany

[4]Photonion GmbH, Hagenower Strasse 73, 19061 Schwerin, Germany

*****Correspondence: thorsten.streibel@uni-rostock.de, Tel.: +49-381-498-6527

SUPPORTING INFORMATION

TABLE OF CONTENT:

Figure A 1. Calibration curves for selected aromatic and polycyclic aromatic hydrocarbons

Figure A 2. Comparison of REMPI-eMIMS Data with REMPI-data obtained by thermogravimetry (TG) coupled to REMPI-TOFMS at an average temperature of 80°C;

Figure A 3. Comparison of REMPI-eMIMS with GC-MS selected polycyclic aromatic hydrocarbons; Calibration curves were used to REMPI-eMIMS measurements

Figure A 4. Extracted REMPI-eMIMS mass spectra of coffee extraction experiments

Figure A 5. Signal responses obtained by REMPI-eMIMS with a non –heated inlet, transfer line and gas inlet using a KrF-Excimer laser (248 nm and 200Hz)

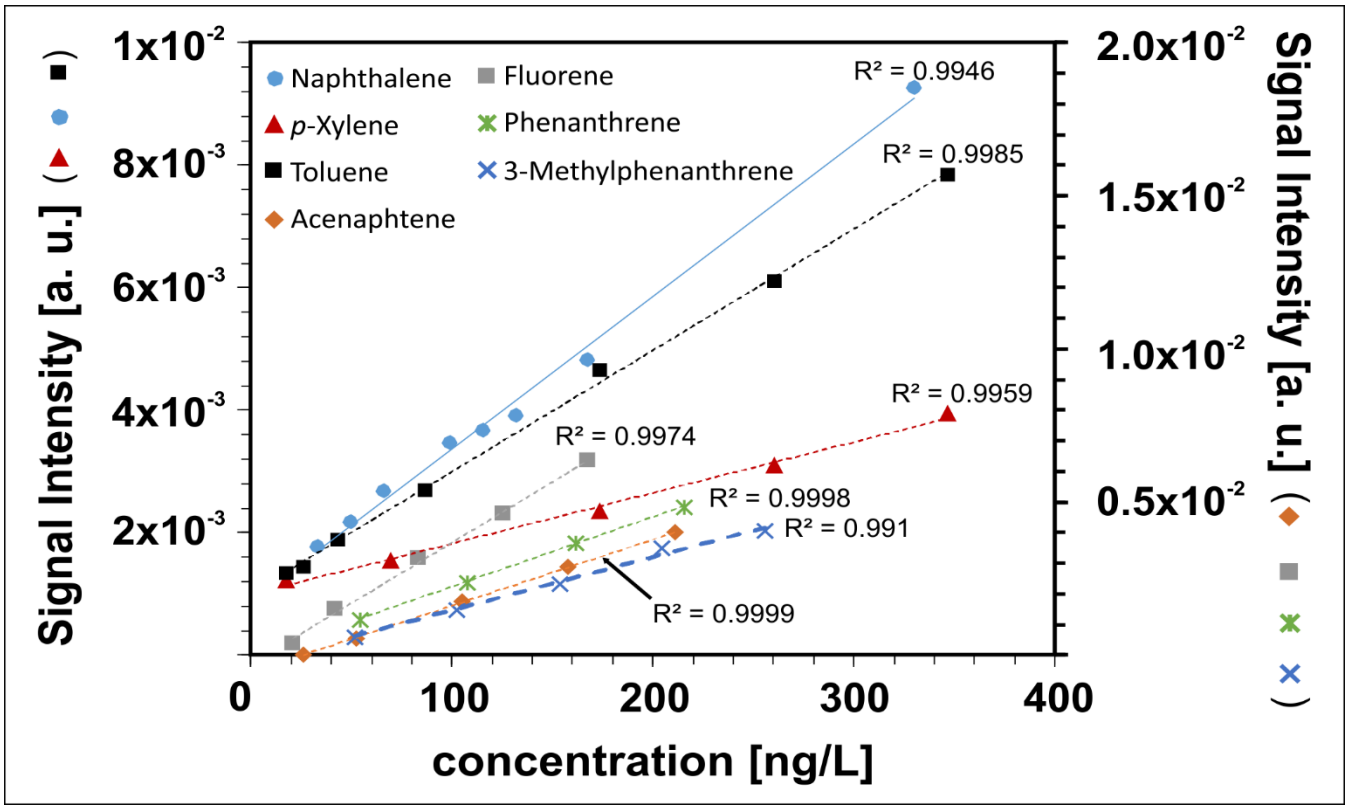

Figure A 1. Calibration curves for selected aromatic and polycyclic aromatic hydrocarbons

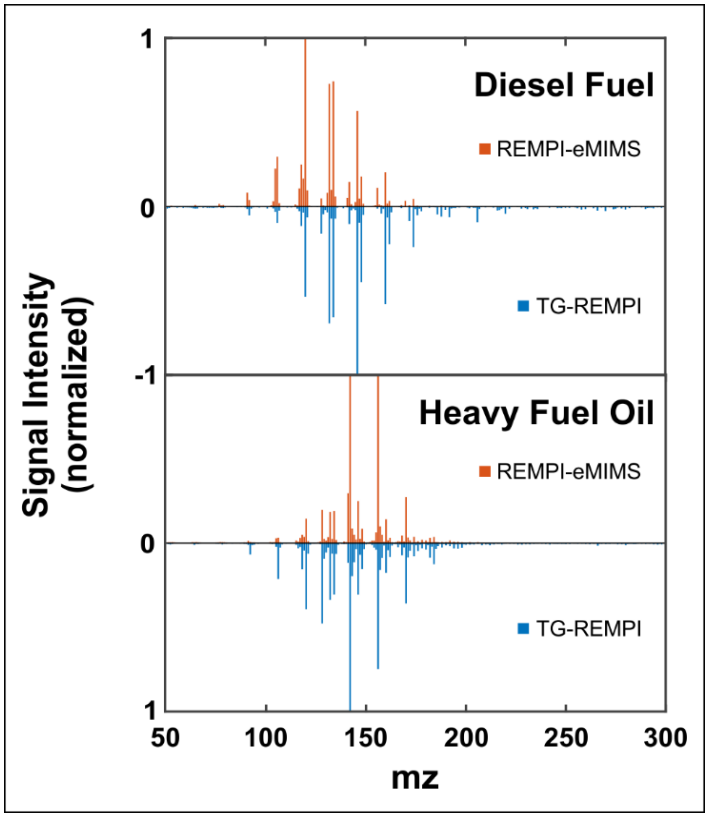

Figure A 2. Comparison of REMPI-eMIMS Data with REMPI-data obtained by thermogravimetry (TG) coupled to REMPI-TOFMS at an average temperature of 80°C;

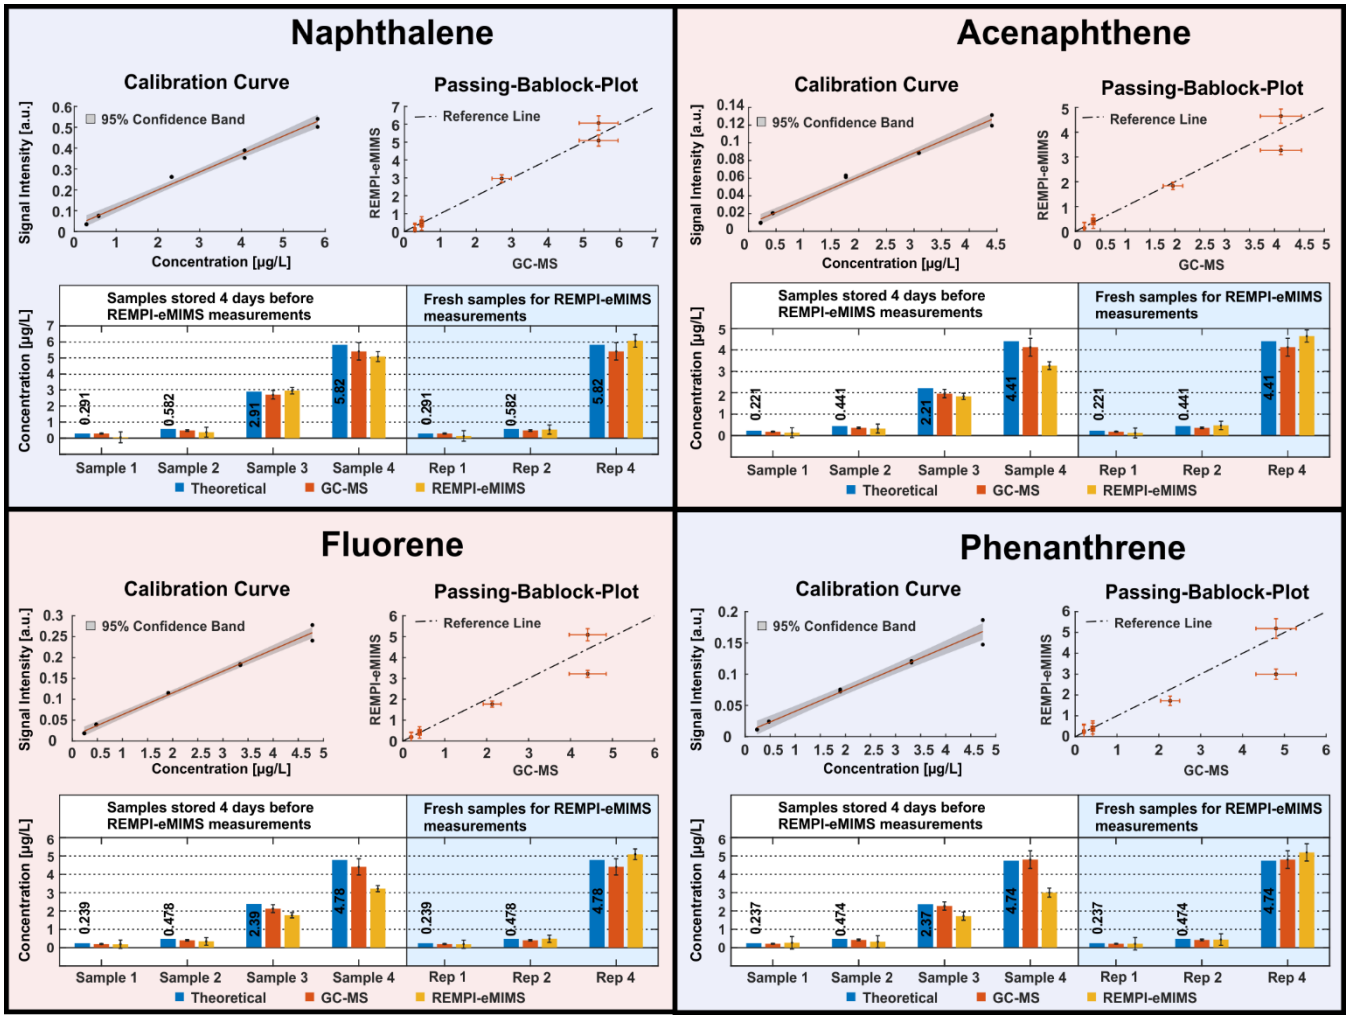

Figure A 3. Comparison of REMPI-eMIMS with GC-MS selected polycyclic aromatic hydrocarbons; Calibration curves were used to REMPI-eMIMS measurements

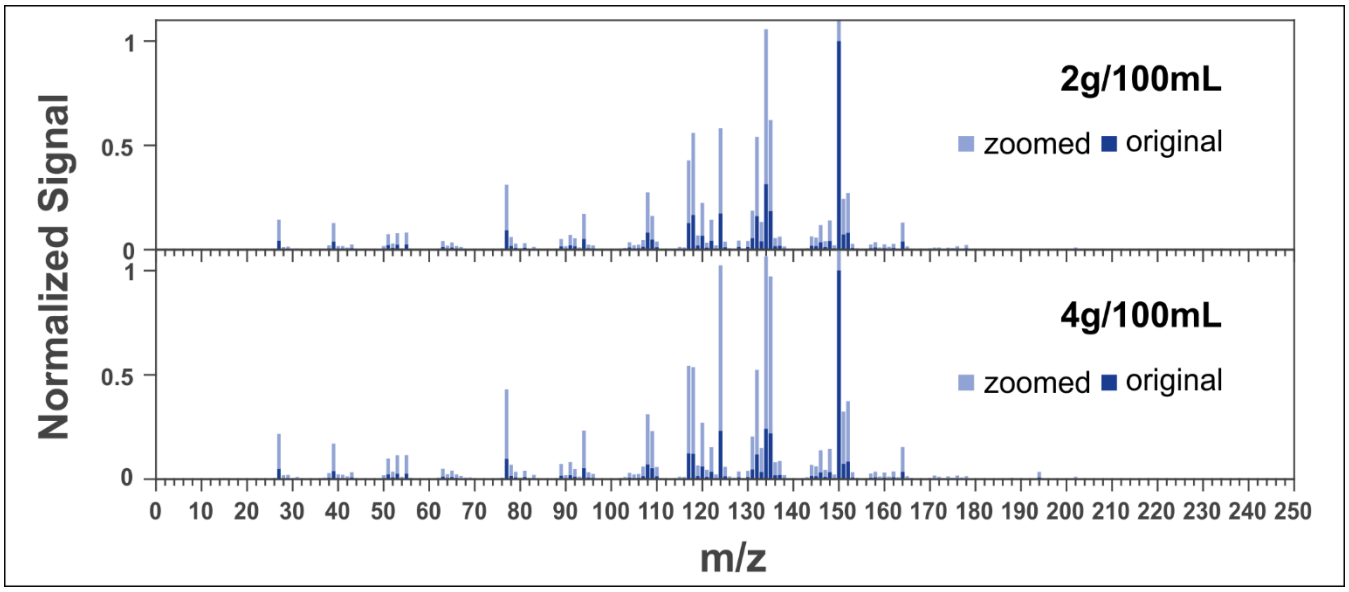

Figure A 4. Extracted REMPI-eMIMS mass spectra of coffee extraction experiments

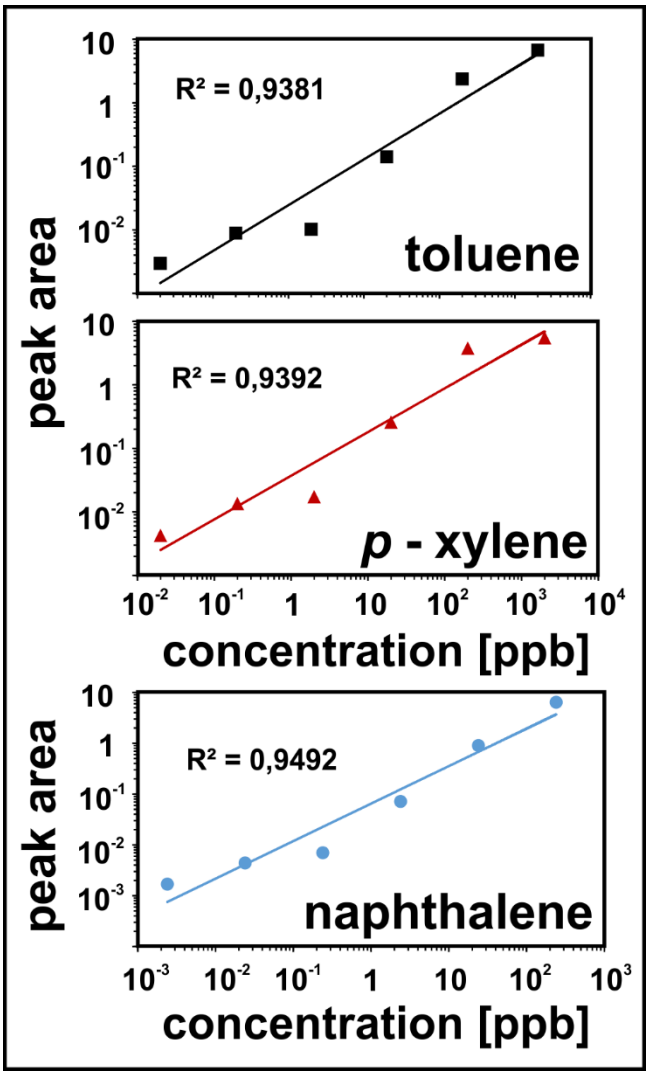

Figure A 5. Signal responses obtained by REMPI-eMIMS with a non –heated inlet, transfer line and gas inlet using a KrF-Excimer laser (248 nm and 200Hz)