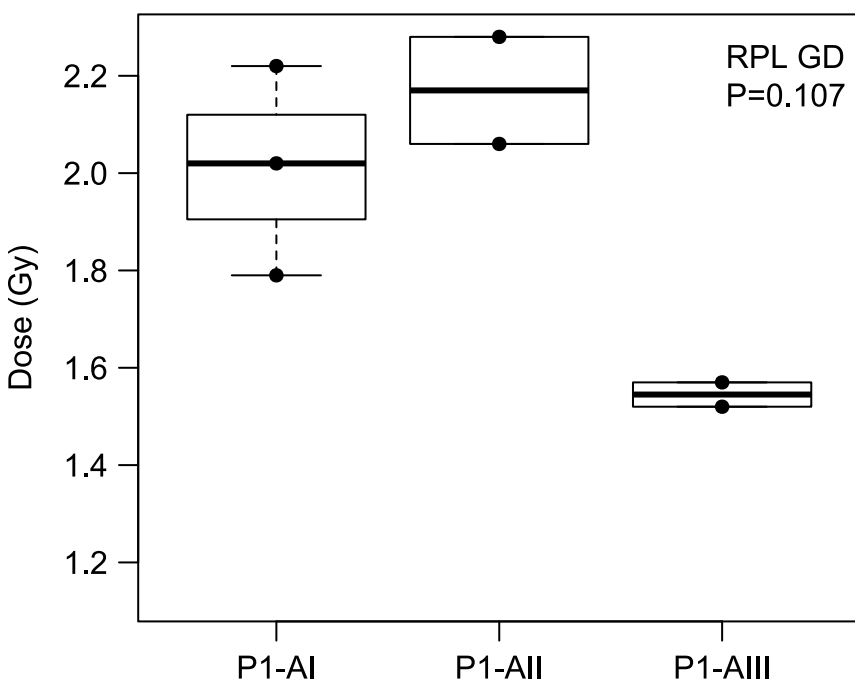
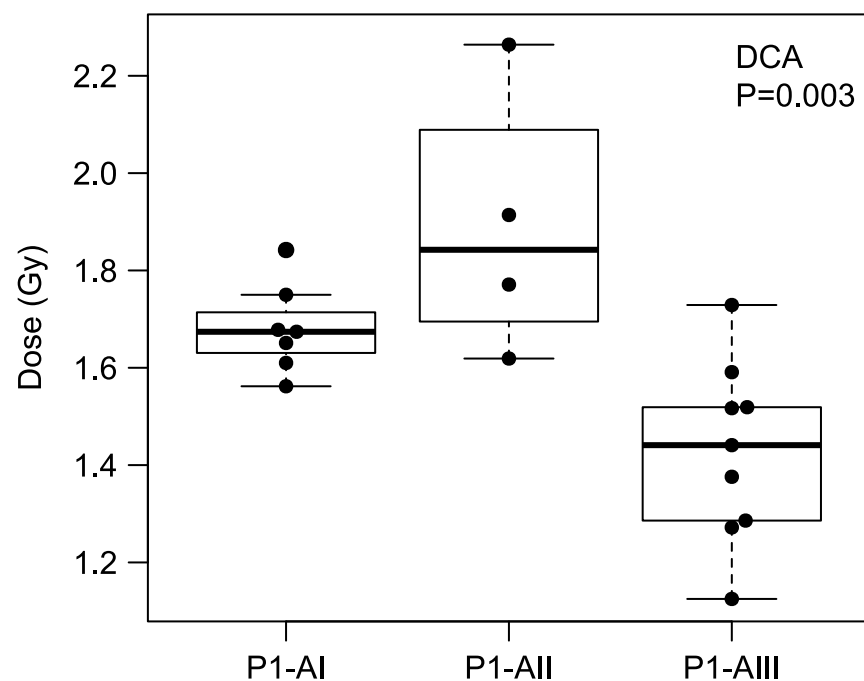
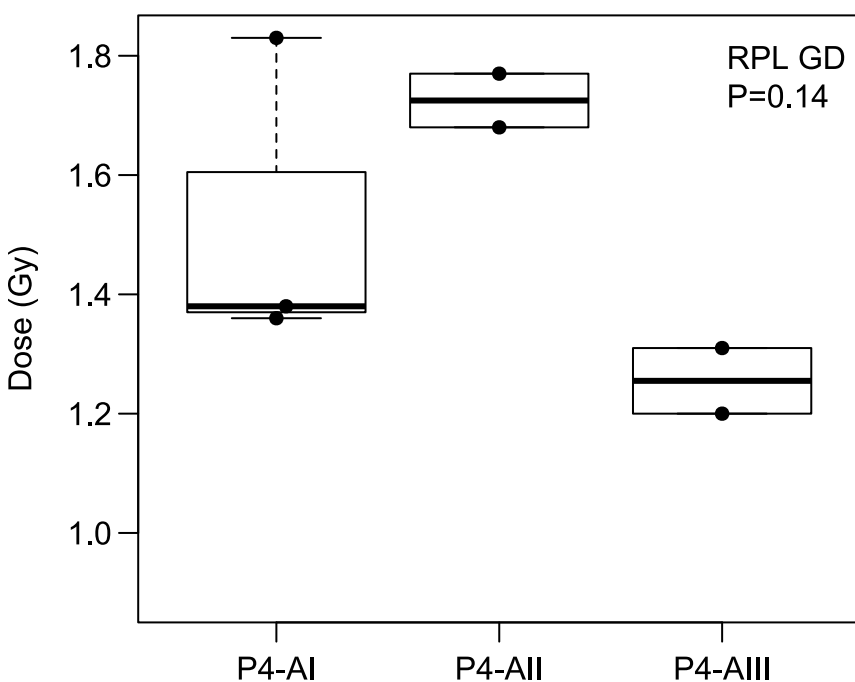
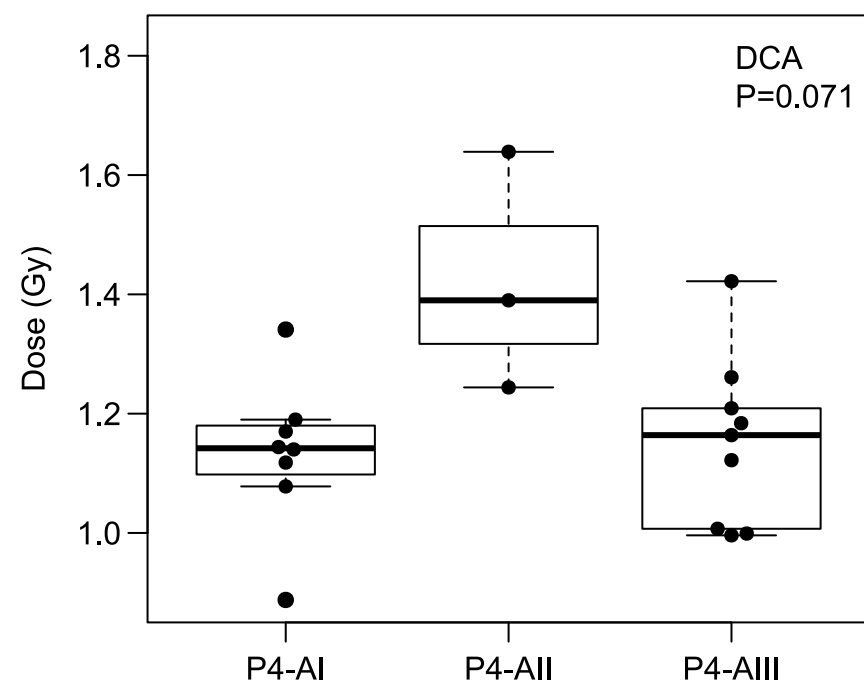


A**B****C****D**

Supplementary Figure 1: Comparison of RPL glass dosimeter and DCA doses between tubes of samples P1-A and P4-A. (A) RPL glass dosimeter reference doses for tubes of sample P1-A. **(B)** Estimated DCA doses for tubes of sample P1-A. **(C)** RPL glass dosimeter reference doses for tubes of sample P4-A. **(D)** Estimated DCA doses for tubes of sample P4-A. P values were estimated by Kruskal-Wallis tests. The results of Lab17 were provided after the blind doses were distributed to the participants and are not shown in this figure.